

General Specifications

Paperless Recorder FX1000



GS 04L21B01-02EN

OVERVIEW

The FX1000 is a Paperless Recorder that displays real-time measured data on a color LCD and saves data on a CompactFlash memory card (CF card^{*1}). It can be hooked up to network via Ethernet, which enables to inform by Email and to monitor on Web site as well as to transfer files by using FTP. Also, it can communicate with Modbus/RTU or Modbus/TCP. It comes with a two, four, six, eight, ten-channel or twelve-channel model. As the input signal, a DC voltage, thermocouple, resistance temperature detector, or contact signal can be set to each channel. The data saved on a CF card or the data transferred via networks can be converted to Lotus 1-2-3, Excel, or ASCII format file, facilitating processing on a PC. Not only this, the Viewer software allows a PC to display waveforms on its screen and to print out waveforms.

*1: On FXs that have a CF card slot (suffix code -4.)



Input Type: DC voltage, 1-5V, thermocouple (TC), resistance temperature detector (RTD), ON/OFF input (DI), and DC current (by adding an external shut resistor)
Measurement range and measurable range:

Signal Input and Alarms

1. Measurement Input

Number of inputs, scan interval, and A/D integration time:

Model	No. of Measurement Channels	Scan Interval	A/D converter integration time
FX1002	2	125 ms, 250 ms	AUTO ^{*1} , 50 Hz, 60 Hz
FX1004	4		
FX1006	6	1 s, 2 s, 5 s	AUTO ^{*1} , 50 Hz, 60 Hz, 100 ms ^{*2}
FX1008	8		
FX1010	10		
FX1012	12		

- *1: AUTO: The FX automatically switches between 50 Hz and 60 Hz depending on the power supply frequency.
- *2: You can only set the integration time to 100 ms on models FX1006 through FX1012. If you set the integration time to 100 ms, you can only set the scan interval to 2 or 5 seconds.
- *1: R, S, B, K, E, J, T, N: IEC584-1 (1995), DIN IEC584, JIS C1602-1995
- *2: W: W-5%Re/W-26%Re (Hoskins Mfg. Co.), ASTM E988-96 (Type C equivalent of OMEGA Engineering Inc.)
- *3: L: Fe-CuNi, DIN43710, U: Cu-CuNi, DIN43710
- *4: WRe: W-3%Re/W-25%Re (Hoskins Mfg. Co.), ASTM E988-96 (Type D equivalent of OMEGA Engineering Inc.)
- *5: Pt100: JIS C1604-1997, IEC751-1995, DIN IEC751-1996
JPt100: JIS C1604-1989, JIS C1606-1989. Measuring current $i = 1 \text{ mA}$ (Pt100, JPt100).
- *6: The range for linear scaling of 1-5V inputs. Burnout detection and non-cut functions are available.
- *7: The detected current value is approximately 10 μA .

Input Type	Range	Measurable Range	
DC voltage	20 mV	-20.000 to 20.000 mV	
	60 mV	-60.00 to 60.00 mV	
	200 mV	-200.00 to 200.00 mV	
	1 V	-1.0000 to 1.0000 V	
	2 V	-2.0000 to 2.0000 V	
	6 V	-6.000 to 6.000 V	
	20 V	-20.000 to 20.000 V	
	50 V	-50.00 to 50.00 V	
1-5V	1 to 5 V ^{*6}	0.800 to 5.200 V	
TC	R ^{*1}	0.0 to 1760.0°C	32 to 3200°F
	S ^{*1}	0.0 to 1760.0°C	32 to 3200°F
	B ^{*1}	0.0 to 1820.0°C	0.0 to 3308°F
	K ^{*1}	-200.0 to 1370.0°C	-328 to 2498°F
	E ^{*1}	-200.0 to 800.0°C	-328.0 to 1472.0°F
	J ^{*1}	-200.0 to 1100.0°C	-328.0 to 2012.0°F
	T ^{*1}	-200.0 to 400.0°C	-328.0 to 752.0°F
	N ^{*1}	-270.0 to 1300.0°C	-454 to 2372°F
	W ^{*2}	0.0 to 2315.0°C	32 to 4199°F
	L ^{*3}	-200.0 to 900.0°C	-328.0 to 1652.0°F
	U ^{*3}	-200.0 to 400.0°C	-328.0 to 752.0°F
	WRe ^{*4}	0.0 to 2400.0°C	32 to 4352°F
RTD	Pt (Pt100) ^{*5}	-200.0 to 600.0°C	-328.0 to 1112.0°F
	JPt (JPt100) ^{*5}	-200.0 to 550.0°C	-328.0 to 1022.0°F
DI	Level	0: Less than 2.4 V. 1: 2.4 V or higher (judged at the 6 V range)	
	Contact ^{*7}	0: Open. 1: Closed (parallel capacitance of 0.01 μF or less)	

Thermocouple burnout:
 Burnout upscale/downscale selectable
 (for each channel).
 Normal: 2 k Ω or less., Burnout: 100 k Ω or
 more (parallel capacitance of 0.01 μ F or less)
 Detection current: Approx. 10 μ A

1-5 range burnout:
 Burnout upscale/downscale selectable
 (for each channel).

Burnout detection:
 Greater than "scale upper limit + 10%
 of scale width" (upscale), or less than
 "scale lower limit – 5% of scale width"
 (downscale)

TC reference junction compensation:
 Internal reference junction compensation
 or external reference junction
 compensation

Filter function:
 Takes the moving average of the input
 values (for each channel).
 Moving average data points: 2 to 400

Computation:
 Difference computation:
 Computable range: DC voltage, TC,
 RTD, and DI

Linear scaling:
 Computable range: DC voltage, TC,
 RTD, and DI
 Scalable range: –30000 to 30000. The
 decimal place is within 4 digits to the
 right of the decimal point.
 Unit: 6 characters or less
 Over value detection: The value can be
 set to over value when \pm 5% of the scale
 range is exceeded.

Square root computation:
 Takes the square root of the input and
 apply linear scaling
 Computable type: DC voltage
 Scalable range and unit: Same as linear
 scaling
 Low-cut: Set the low-cut value in the
 range of 0.0% to 5.0% of the span.
 Over value detection: Same as linear
 scaling

1-5V:
 Computable range: 1 to 5 V
 Scalable range and unit: Same as linear
 scaling
 Low-cut: The low-cut point is fixed to the
 span lower limit.
 Over value detection: Same as linear
 scaling

2. Alarms

Number of alarms:
 Up to 4 alarms (levels) per measurement
 channel

Alarm type:
 High limit, low limit, difference high limit,
 difference low limit, high limit on rate-of-
 change alarm, low limit on rate-of-change
 alarm, delay high limit, and delay low limit

Alarm delay time:
 1 to 3600 s (for each channel)

Rate-of-change calculation interval of rate-of-change alarms:
 1 to 32 times the scan interval (common
 to all channels)

Alarm output:
 Output to the internal switch
 Number of internal switches: 30
 Internal switch operation: AND/OR
 operation selectable

Hysteresis:
 High and low limit alarm: 0.0 to 5.0% of
 the span (common to all channels)
 Difference high and low limit alarms:
 0.0 to 5.0% of the span (common to all
 channels)

Display:
 Displays the status on the respective
 operation screen and an alarm icon on
 the status display section when an alarm
 occurs.
 Display operation: Hold or not hold the
 display until the alarm acknowledge
 operation.

Alarm hide function (alarm no logging function):
 Not display alarms nor record to the alarm
 summary (for each channel)

Alarm information:
 Displays a log of alarm occurrences on
 the alarm summary.

■ Display

1. Display

Display*: 5.7-inch TFT color LCD (240 × 320 dots)
 Brightness: 8 levels
 Backlight saver function:
 Dim or turn off the LCD backlight if there
 is no key operation for a specified time.

* A section of the LCD monitor may contain
 pixels that are always on or off. The brightness
 of the LCD may also not be uniform due to
 the characteristics of the LCD. This is not a
 malfunction.

2. Displayed Information

Display groups:
 Assign channels to groups on the trend
 display, digital display, and bar graph
 display and display.
 Number of groups: 10
 Number of channels that can be assigned to each group:
 Up to six

Display color:
 Channel: Select from 24 colors
 Background:
 White or black (excludes the Overview
 display. See the item on the Historical
 trend display for information on that
 display.)

Trend display:
 Waveform line width
 Select from 1, 2, and 3 dots

Display method
 Orthogonal axis display with time axis
 (T) and measured value axis (Y)

Layout: Vertical, horizontal, or wide

Trend intervals:
 15 s, 30 s, 1 min, 2 min, 5 min,
 10 min, 15 min, 20 min, 30 min, 1 h, 2
 h, 4 h, or 10 h/div for the FX1002 and
 FX1004.
 30 s, 1 min, 2 min, 5 min, 10 min,
 15 min, 20 min, 30 min, 1 h, 2 h, 4 h,
 or 10 h/div for the FX1006, FX1008,
 FX1010, and FX1012.

Switchable to the secondary trend interval.

Scale Display a scale for each channel.
 Current value bar graph, color scale
 band, and alarm point marks can be
 displayed on the scale.

Others Grid (divisions: 4 to 12), trip line (line
 width: 1, 2, or 3 dots), message, zone
 display, and partial expanded display

Digital Display: Displays measured values numerically

Update rate 1 s (scan interval if the scan interval
 is greater than 1 s)

Bar graph display:
 Displays the measured value on a bar graph

Direction Vertical or horizontal

Base position End or center

Update rate 1 s (scan interval if the scan interval
 is greater than 1 s)

Scale Display a scale for each channel
 Color scale band, and alarm point marks
 can be displayed on the scale.

Historical trend display:
 Redisplays the display data or event data
 in the internal memory or external storage
 medium*

* On FXs that have a CF card slot (suffix code -4.)
 or USB interface (USB1 option).

Display formats
 All screen or half screen (only when the
 display data is being redisplayed)

Time axis operation
 The time axis can be reduced or
 expanded, and data can be displayed
 continuously.

Add message
 Messages can be added.

Background color
 Select from white, cream, black, or light gray.

Overview Display:
 Displays the measured values of all
 channels and the alarm statuses.

Information display:
 Alarm summary display
 Displays a log of up to 1000 alarms.
 Specify an alarm with the cursor and
 jump to the corresponding section on
 the historical trend display.

Message summary display
 Time and content of up to 450
 messages (including 50 add messages)
 Specify a message with the cursor and
 jump to the corresponding section on
 the historical trend display.

Memory summary display
 Displays the information of the data in
 the memory.
 Specify a file with the cursor and jump
 to the corresponding section on the
 historical trend display.
 Save the data in the internal memory to
 the external storage medium using keys.

* On FXs that have a CF card slot or USB interface
 (USB1 option)

Report (/M1, /PM1, and /PWR1)
 Displays report data from the internal
 memory

Stacked bar graph (/M1, /PM1, and /PWR1)
 Displays the report data of each report
 group in a stacked bar graph.

Display formats:
 H+D (hourly data is used for the
 display), Day+Week (daily data is used
 for the display), D+M (daily data is used
 for the display)

Report groups:
 Report channels are arranged in groups
 of six starting with the first report
 channel (R01). The group arrangements
 are fixed.

Scale/grid: Fixed at four divisions

Update interval: 1 s
 The report data of the channels in the
 specified group is displayed in a stacked
 bar graph.
 However, only channels that have the
 same unit of measurement as the first
 channel in the group are displayed.

Status Display
 Relay status display: Displays the ON/
 OFF status of the alarm output relay and
 internal switch.

Modbus client status (/C7):
 Displays the communication status on
 the Modbus client

Modbus master status (/C2, /C3):
 Displays the communication status on
 the Modbus master

Log display:
 Displays the login log, error log,
 communication log (/C2, /C3, and /C7),
 FTP log (/C7), Web log (/C7), e-mail log (/C7),
 SNTP log (/C7), and DHCP log (/C7)

System information display:
 Displays the number of measurement
 and computation channels, options, MAC
 address, firmware version, and internal
 memory capacity.

Network information display (/C7):
 Displays the FX network setup information

3. Other Displayed Information

Tag display: Tag
 Up to 16 characters

Message: Write messages to the trend display.
 Number of messages 100
 Maximum number of saved messages 400
 Character Up to 32 characters

Write method
 Write a preset message or write an
 arbitrary message on the spot.

Write destination
 Select only the displayed group or all
 groups.

Auto message
 Write a message when the FX recovers
 from a power failure while memory
 sampling is in progress.
 Write a message when the trend interval
 is switched during memory sampling.

Add message:
 Write messages to the past data positions.
 Message The same as the "Message" item above
 Maximum number of saved messages 50

Status display section:
 Displays the FX status in the upper part of the display

Displayed contents
 Year, month, day, time, displayed group name/display name, user name (when the login function is in use), batch name (when the batch function is in use), internal memory status, external storage medium status (on FXs with a CF card slot), alarm status, function usage status (key lock, computation function—/M1, /PM1, /PWR1), and e-mail (/C7)

Auto switching of displayed groups:
 Switches the display group at a given interval.
 Interval: Select from the available settings between 5 s and 1 min.

Default display:
 Specify the display to be shown automatically when keys are not operated.
 Time until the display switches: Select from the available settings between 1 min and 1 h.

Display language:
 Select from English, Japanese, German, French, Chinese, Italian, Spanish, Portuguese, Russian, and Korean.

Display selection menu customization:
 Show/hide and change the positions of each item in the display menus and sub menus
 Insert/delete separators.

Function menu customization:
 Show/hide and change the display positions of each item.

■ Data Saving Function

1. Configuration

Internal memory:
 Temporarily saves various types of data.
 Medium Flash memory

External storage medium (on FXs with a CF card slot):
 Medium CF card
 Format FAT32 or FAT16

2. Data Type

FX data types and file name extensions

Data Type	Extension	Notes
Display data	.DAD	
Event data	.DAE	
Manual sampled data	.DAM	
Screen image data	.PNG	
Setup data	.PDL	
Report data	.DAR	/M1, /PM1, and /PWR1

3. Display Data and Event Data

Internal memory:
 File storage capacity 400 MB
 Number of files Up to 400
 Operation FIFO (First In First Out)

Display data:
 Target Measurement/computation channel
 Sampling intervals Synchronized to the trend interval.
 Content Maximum and minimum value per sampling interval
 File size Up to 8 MB
 Data format Binary
 Recording Records data at all times.

Event data:
 Target Measurement/computation channel.
 Sampling interval Determined by the sample rate.
 125 ms, 250 ms, 500 ms, (FX1002 and FX1004 only)
 1 s, 2 s, 5 s, 10 s, 30 s, 1 min, 2 min, 5 min, or 10 min
 The sampling interval cannot be shorter than the scan interval.
 Content Data per sampling interval
 File size Up to 8 MB
 Data format Binary
 Mode Free: Records data at all times.
 Trigger: Starts recording data when a certain event occurs and records for the specified interval.

Combinations of saved data:
 Display data only, event data only, or display data and event data.
 Sampled Data Size
 • Data Size of Display Data and Event Data

Channel	Display Data	Event Data
Measurement channel	4 bytes/channel	2 bytes/channel
Computation channel	8 bytes/channel	4 bytes/channel

Time data common to all channels is added for each sample.

Time data	8 bytes/sample
-----------	----------------

• Data Size per Sample

Display Data
 (Number of measurement channels×4 bytes) + (number of computation channels×8 bytes) + 8 bytes (time data)

Event Data
 (Number of measurement channels×2 bytes) + (number of computation channels×4 bytes) + 8 bytes (time data)

Sampling Time for a Single File (8 MB)
 The sampling time for a single file (8 MB) is calculated as follows:
 Number of samples × sampling interval.
 The number of samples is calculated as follows:
 8 MB/(the data size per sample)

Only Display Data

If the display data from the 12 measurement channels and the 24 computation channels is recorded at the trend interval of 30 min/div and the display data's sampling interval is 60 seconds:

Number of samples
 = 8 MB/(8 bytes + 12 × 4 bytes + 24 × 8 bytes) = Approximately 32,258 samples
 Sampling time per file (8 MB)
 = 32,258 × 60 seconds = 1,935,480 seconds = Approximately 22 days

Only Event Data

If the event data from the 12 measurement channels and the 24 computation channels is recorded at the sampling interval of 1 second:

Number of samples
 = 8 MB/(8 bytes + 12 × 2 bytes + 24 × 4 bytes) = Approximately 62,500 samples
 Sampling time per file (8 MB)
 = 62,500 × 1 seconds = 62,500 seconds = Approximately 17 hours

Display data and event data

Display data file size = 8 MB
 Event data file size = 8 MB

You can use these figures to calculate the sampling time per file in the same manner as was used for the case of "Only Display Data" or "Only Event Data." You can save multiple files such as those described above to the internal memory or to an external memory device (the number of files that can be stored is limited by the size of the internal memory or external memory device).

Calculation Examples of the Sampling Time for a Single File (8 MB)

Examples of the sampling time for a single file (8 MB) are shown below. You cannot actually set recording conditions so that the sampling time exceeds 31 days. If the sampling time exceeds 31 days, the file will be divided even if it is not 8 MB in size.

4 Measurement Channels and No Computation Channels
 Display data file

Trend interval (time/div)	15 s	30 s	1 min	2 min	5 min	10 min
Sampling interval	0.5 s	1 s	2 s	4 s	10 s	20 s
Sampling time (approx.)	42.7 hours	3 days	7 days	14 days	35 days (-> 31 days)	71 days (-> 31 days)

Event data file

Sampling interval	125 ms	0.5 s	1 s	2 s	5 s	10 s
Sampling time (approx.)	15.4 days	2 days	5 days	10 days	25 days	51 days (-> 31 days)

12 Measurement Channels and 24 Computation Channels
 Display data file

Trend interval (time/div)	30 s	1 min	5 min	10 min	30 min	1 hour
Sampling interval	1 s	2 s	10 s	20 s	1 min	2 min
Sampling time (approx.)	9 hours	17.9 hours	3 days	7 days	22 days	44 days (-> 31 days)

Event data file

Sampling interval	1 s	2 s	5 s	10 s	30 s	1 min
Sampling time (approx.)	17.3 hours	1.4 days	3.6 days	7.2 days	21 days	43 days (-> 31 days)

4. Manual Sampled Data

Item: Measured value at an arbitrary time
 Maximum number of data values that the internal memory can store: 400
 Data format: Text

5. Report Data (/M1, /PM1, and /PWR1)

Item: Report at each scheduled time of report
 Maximum number of reports that the internal memory can store: 100
 Data format: Text

6. Snapshot Data

Item: Displayed screen image data
 Data format: PNG
 Output destination: CF card or communication output

7. Saving Data to the External Storage Medium (On FXs with a CF card slot or the /USB1 option)

Data Saving: Saves the data in the internal memory to the external storage medium.

Manual save: Saves when the external storage medium is inserted with a key operation.

Auto save*
 Display data: Every file save interval
 Event data: Every data length

Manual sampled data:
 When manual sampling is executed.

Report data: When report is created.
 Snapshot data: When a snapshot is taken

Auto save operation*
 Select "save data only if there is sufficient free space on the CF card" or "constantly retain the most recent data files in the CF card (media FIFO)."

* This is only valid on FXs that have a CF card slot.
 File name: Select from "sequence number+user-assigned string+date," "sequence number+user-assigned string," or "sequence number+batch name."

Save destination
 Auto save: CF card (only valid on FXs that have a CF card slot (suffix code -4).)

Manual save: CF card (only valid on FXs that have a CF card slot (suffix code -4) or USB flash memory (/USB1 option)
Directory name: Specify using up to 20 characters.

8. Setup Data (On FXs with a CF card slot or the /USB1 option)

Item: FX setup data
Data format: Binary
File name: Specify using up to 32 characters.
Output/read destination (for saving/loading):
CF card or USB flash memory (/USB1)

9. Data File Loading (On FXs with a CF card slot or the /USB1 option)

Function: Load and show the display data or event data in a CF card or USB flash memory (/USB1).

10. Miscellaneous

Header comment:
Add up to 50 characters of comment to display data, event data, manual sampled data, or report data file.

■ Other Standard Functions

1. Event Action Function

Event action:
Execute a specified operation when a given event occurs.
Number of settings: 40
Events: Remote control input, etc.
Timer Number of timers: 4
Match time timer Number of timers: 4
Action: Specify memory start/stop, alarm ACK, etc.
There are limitations on the combinations of events and actions.

2. Security Function

Key lock function:
Limitations to key operation, access to the external storage medium (on FXs with a CF card slot or the /USB1 option), and various operations
Login function:
Only registered users can operate the FX.
System administrators
5 administrators (with total operation access)
Users
30 users (with access to operations based on their user access rights)
User access rights setting
Limitations to key operation, access to the external storage medium (on FXs with a CF card slot or the /USB1 option), and various operations
Automatic logout function
Users are logged out automatically if there are no key operations for the specified period of time.

3. Time Related Functions

Clock: With a calendar function
Accuracy ±50 ppm (0 to 50°C); does not include the delay (1 second or less) that occurs when the power is turned on
Time setting: Set by way of key operations, communication commands (/C2, /C3, and /C7), the event action function, or the SNTP client function (/C7)
Time adjustment method:
While memory sampling
Corrects the time by 40 ms for each second.
Limit in which the time is gradually adjusted: Select from the available settings between 10 s and 5 min.
If the time is outside the limit, the time is immediately corrected.
Cannot be used after hour 0 on January 1st, 2038.
While memory sampling is stopped
Immediately change the time.
DST: The date/time for switching between standard time and DST can be specified.
Time zone: Sets the time difference from GMT.
Date format:
Select YYYY/MM/DD, MM/DD/YYYY, DD/MM/YYYY, or DD.MM.YYYY.

4. Types of Characters That Can Be Handled

Characters:
Alphabet characters, numbers, and symbols (limitation exists)
European special character and Cyrillic can be entered via communication command and DAQSTANDARD software.

5. Miscellaneous

Decimal point type: Period or comma

6. Batch Function

Function: Data management using batch names.
Enter text fields and batch comments in the data file.
Batch name:
Added to the file name of the display data and event data.
Structure Batch number (up to 32 characters) + lot number (up to 8 digits)
Text field: Adds text to the display data and event data. There are 8 available text fields.
Up to 20 title characters and 30 other characters can be entered per field.
Batch comment:
Adds text to the display data and event data. Up to 3 comments with 50 characters or less.

■ Options

1. Alarm Output Relay (/A1, /A2, /A3, and /A4A)

- Action: Outputs relay contact signals from the terminals on the rear panel when alarms occur.
- Number of outputs:
2 (/A1), 4 (/A2), 6 (/A3), and 12 (/A4A)
- Relay contact rating:
250 VAC (50/60 Hz)/3 A, 250 VDC/0.1 A (for resistance load)
- Output format:
2 (/A1), 4 (/A2), 6 (/A3): NO-C-NC, and 12 (/A4A): NO-C
- Relay operation:
Energized/deenergized, AND/OR, hold/non-hold, and reflash settings are selectable.

2. RS-232 Interface (/C2) and RS-422A/485 Interface (/C3)

- Connection:
EIA RS-232(/C2) or EIA RS-422A/485(/C3)
- Protocol: Dedicated protocol or Modbus protocol
- Synchronization: Start-stop synchronization
- Transmission mode (RS-422A/485):
Four-wire half-duplex multi-drop connection (1:N (N = 1 to 32))
- Data rate: 1200, 2400, 4800, 9600, 19200, or 38400 bps
- Data length: 7 or 8 bits
- Stop bit: 1 bit
- Parity: Odd, even, or none
- Handshaking:
Off:Off, XON:XON, XON:RS, and CS:RS
- Communication distance (RS-422A/485): 1200 m
- Modbus master:
Reading information such as measured data from other instruments and writing information to registers
- Modbus slave:
Reading data from measurement and computation channels (/M1, /PM1, and /PWR1)
Reading and writing communication input data (/M1, /PM1, and /PWR1)
Some control commands such as memory start

3. Ethernet Communication Interface (/C7)

- Electrical and mechanical specifications:
Conforms to IEEE 802.3 (Ethernet frames conform to the DIX specification).
- Medium: Ethernet (10BASE-T)
- Protocol: Dedicated protocol as well as the TCP, IP, UDP, ICMP, ARP, DHCP, HTTP, FTP, SMTP, SNTP, and Modbus protocols
- E-mail client:
Automatically send e-mail at specified times.
- FTP client: Automatically transfer the following types of data files to the FTP server:
Display data, event data, screen image (snapshot) data, and report data (/M1, /PM1, and /PWR1)

- FTP Server:
Moving and deleting files on the FX, managing directories, and generating file lists
- Web server:
Displaying the FX screen on a Web browser
- SNTP client:
Setting the FX time to the results of an SNTP server query
Cannot be used after hour 0 on January 1st, 2036.
- SNTP server: Generating the FX's time.
Time resolution: 5 ms
Cannot be used after hour 0 on January 1st, 2036.
- DHCP client:
Automatically obtain the network address settings from the DHCP server.
- Modbus client:
Reads data from another device and writes to the registers.
- Modbus server:
Reading data from measurement and computation channels (/M1, /PM1, and /PWR1)
Reading and writing communication input data (/M1, /PM1, and /PWR1)
Some control commands such as memory start. Modbus client access limitations.
- Setting/Measurement server:
Using the dedicated protocol control, and configure the FX, and generate data from the FX.
- Maintenance/test server:
Outputs connection information and network information.
- Instrument information server:
Generating the information (such as the serial number and model name) of the connected FX.

4. FAIL/Status Output Relay (/F1)

- FAIL output: Relay contact output on CPU error
Relay operation
Energized during normal operation and de-energized on system error.
- Status output:
Output a relay contact signal when a selected condition occurs.
A combination of the following conditions can be selected:
Low memory, memory failure, media error, A/D hardware error, burnout detection, communication error (Modbus master or client communication error), memory sampling stop.
- Relay operation:
Relay is energized when a condition occurs.
- Relay contact rating:
250 VAC (50/60 Hz)/3 A, 250 VDC/0.1 A (for resistance load)

5. Computation Function (including the report function) (/M1)

Number of computation channels:
 FX1002 and FX1004: 12 channels (101 to 112)
 FX1006, FX1008, FX1010, and FX1012: 24 channels (101 to 124)

Operation:
 General arithmetic operations:
 Four arithmetic operations, square root, absolute, common logarithm, natural logarithm, exponential, and power

Relational operations: <, ≤, >, ≥, =, and ≠

Logic operations: AND, OR, NOT, and XOR

Statistical operations: TLOG and CLOG

Special operations:
 PRE, HOLD, RESET, and CARRY

Conditional operation: [a?b:c]

Computation accuracy:
 Double-precision floating point

Data that can be used:
 Channel data
 Measurement and computation channels

Constants 60 constants

Communication input data 24

Remote control input status 0/1 (/R1)

Pulse input Counts the number of pulses (/PM1)

Status input Internal switch, alarm output relay (/A[] and /A4A), flags

Rolling average:
 Performs moving average on the computed results.

Measurement range: -9999999 to 99999999
 Decimal place: 0 to 4 digits to the right of the decimal point

Unit: Up to 6 characters in length
 Sum scales: Off, /s, /min, /h, /day

Alarms: High limit, low limit, delay high limit, and delay low limit
 Hysteresis: High and low limit alarm: 0.0% to 5.0% of the span.

Display: Same as the measurement channels

Data saving: Same as the measurement channels

Report function:
 Number of report channels: 12 or 24 (same as the number of computation channels)

Computation types:
 Average, maximum, minimum, sum, or instantaneous value

Report types:
 Hourly, daily, hourly + daily, daily + weekly, daily + monthly

6. 3-Wire Isolated RTD Input (/N2)

Input terminal:
 All the RTD input terminals (A, B, and b) are isolated on each channel.
 Applies to the FX1006, FX1008, FX1010, and FX1012

Note: On the FX1002 and FX1004 standard models, the A, B, and b terminals are already isolated on each channel.

7. Extended Input (/N3F)

Measurement/display accuracy: Under standard operating conditions

Input Type		Measuring Range		Measurement Accuracy	Max. Resolution
Thermocouple	Kp vs Au7Fe	0.0 to 300.0 K	0 to 20 K	Within ±4.5 K	0.1 K
			20 to 300 K	Within ±2.5 K	
	PLATINEL	0.0 to 1400.0°C	±(0.25% of rdg + 2.3°C)		0.1°C
	PR40-20	0.0 to 1900.0°C	0 to 450°C	Accuracy not guaranteed	
			450 to 750°C	±(0.9% of rdg + 3.2°C)	
			750 to 1100°C	±(0.9% of rdg + 1.3°C)	
			1100 to 1900°C	±(0.9% of rdg + 0.4°C)	
	NiNiMo	0.0 to 1310.0°C	±(0.25% of rdg + 0.7°C)		
	W/WRe26	0.0 to 2400.0°C	0 to 400°C	±15.0°C	
			400 to 2400°C	±(0.2% of rdg + 2.0°C)	
Type N (AWG14)	0.0 to 1300.0°C	±(0.2% of rdg + 1.3°C)			
XK GOST	-200.0 to 600.0	-200 to -100°C	±(0.25% of rdg + 1.0°C)		
		-100 to 600°C	±(0.25% of rdg + 0.8°C)		
RTD*1	Ni100 (SAMA)	-200.0 to 250.0°C	±(0.15% of rdg + 0.4°C)		
	Ni100 (DIN)	-60.0 to 180.0°C	±(0.15% of rdg + 0.4°C)		
	Ni120	-70.0 to 200.0°C	±(0.15% of rdg + 0.4°C)		
	Pt100 GOST	-200.0 to 600.0°C	±(0.15% of rdg + 0.3°C)		
	Cu100 GOST	-200.0 to 200.0°C	±(0.15% of rdg + 0.3°C)		
	Cu50 GOST	-200.0 to 200.0°C	±(0.4% of rdg + 0.5°C)		
	Pt200 (WEED)	-100.0 to 450.0°C	±(0.3% of rdg + 0.6°C)		

*1: Measuring current i = 1 mA

Input source resistance:

Thermocouple input: 2 k Ω or less

RTD input: 1 Ω or less per wire (The resistance of all three wires must be equal).

Ambient temperature influence (with temperature variation of 10°C):

TC input $\pm(0.1\%$ of rdg + 0.05% of range) or less, excluding the error of reference junction compensation

RTD input $\pm(0.2\%$ of range + 2 digits) or less

Input source resistance:

TC input With variation of +1 k Ω : ± 10 μ V or less

RTD input With variation of 1 Ω per wire (resistance of all three wires must be equal): $\pm(0.1\%$ of rdg + 1 digit) or less
With maximum difference of 100 m Ω between wires: Approx. 1 °C

8. Remote Control (/R1)

Number of input terminals: 8

Input type: Isolated from the main circuitry through a photocoupler, built-in isolated power supply for the input terminals, and shared common.

Input type and signal level:

Voltage-free contact

Contact closed at 200 Ω or less and contact open at 100 k Ω or greater.

Open collector

ON voltage: 0.5 V or less (sink current 30 mA or more), leakage current when OFF: 0.25 mA or less

Allowable input voltage: 5 VDC

Signal type: Level or edge (250 ms or more)

Action: Executes a specified action by applying a given signal to the remote signal input terminal.

Action assignment: Set using the event action function

9. 24 VDC Transmitter Power Supply (/TPS2 and /TPS4)

Number of loops: 2 (/TPS2) or 4 (/TPS4)

Output voltage:

22.8 to 25.2 VDC (under rated load current)

Rated output current: 4 to 20 mADC

Max. output current:

25 mADC (overcurrent protection operation current: approx. 68 mADC)

Allowable conductor resistance:

$RL \leq (17.8 - \text{minimum transmitter operation voltage})/0.02$ A
where 17.8 V is the result obtained by subtracting the maximum drop voltage of 5 V when the load shunt resistance is 250 Ω from the minimum output voltage of 22.8 V

Max. length of wiring:

2 km (when using the CEV cable)

Insulation resistance:

20 M Ω or more at 500 VDC between output terminal and ground

Dielectric strength:

500 VAC (50/60 Hz, I = 10mA) for one minute between output terminal and ground

500 VAC (50/60 Hz, I = 10mA) for one minute between output terminals

10. USB Interface (/USB1)

USB port: Complies with Rev. 1.1 and host function

Number of ports: 1 (front panel)

Power supply: 5 V, 500 mA

Connectable devices:

Only connect the devices listed below to prevent damage to the devices.

Keyboard Complies with HID Class Ver. 1.1
104 keyboard/89 keyboard (US) and
109 keyboard/89 keyboard (Japanese)
Number of connectable units: 1

External medium

USB flash memory

Does not guarantee the operation of all USB flash memories.

External medium such as a hard disk, ZIP, MO, and optical discs are not supported.

Number of connectable units: 1

11. Pulse Input (/PM1)

Pulse input:

Number of inputs

3 (8 when using the remote control input terminals)

Input type Isolated from the main circuitry through a photocoupler and built-in isolated power supply for the input terminals.
Shared common for pulse inputs.

Input type and signal level

Voltage-free contact

Contact closed at 200 Ω or less and contact open at 100 k Ω or greater

Open collector

ON voltage: 0.5 V or less (sink current 30 mA or more), leakage current when OFF: 0.25 mA or less

Counting Counts the rising edges of pulses.

For voltage-free contact input:

Contact open to contact close

For open collector:

Voltage level of the terminal H from high to low

Allowable input voltage 30 VDC

Max. sampling pulse period 100 Hz

Minimum detected pulse width

5 ms or more for both low (closed) and high (open)

Pulse detection period Approx. 3.9 ms (256 Hz)

Pulse measuring accuracy ± 1 pulse

Pulse count interval Scan interval or 1 s

Miscellaneous

Pulse input terminals can be used as remote control input terminals, isolated from remote control input terminals

Remote control:

Number of inputs: 5. Same as remote control (/R1) for the other specifications

Computation function:

Same as the computation function (/M1)

12. Calibration Correction (/CC1)

Calibration correction method:

Corrects the measured value of each channel using segment linearizer approximation.

Number of segment points: 2 to 16 (including the start and end points)

13. DC/AC 24 V Power Supply (/P1)

Rated supply voltage:
 24 VDC and 24 VAC (50/60Hz)
 Allowable power supply voltage range:
 21.6V to 26.4 VDC/AC
 Insulation resistance:
 Between power terminal and earth: 20 MΩ or greater at 500 VDC.
 Withstand voltage:
 Between power terminal and earth: 500 VAC at 50/60 Hz for one minute
 Rated power supply frequency (for AC): 50/60 Hz
 Allowable power supply frequency range (for AC):
 50 Hz ±2%, 60 Hz ±2%
 Power supply fluctuation:
 With variation within 21.6 to 26.4 VDC/AC: ±1 digit or less
 Power supply frequency fluctuation (for AC):
 With variation of ±2 Hz from rated power supply frequency: ±(0.1% of rdg+1 digit) or less
 Rated power consumption:
 18 VA (for DC), 30 VA (for AC)
 Power consumption:

Supply voltage	LCD backlight off	Normal	Maximum
24 VDC	5 VA	7 VA	18 VA
24 VAC (50/60Hz)	8 VA	12 VA	30 VA

14. Log Scale (/LG1)

Function: A logarithmic voltage that has been converted from a physical value is applied to the FX, and then the FX's Log scale (logarithmic scale) is used to display and record the physical value.
 Input type: Log input: Logarithmic input (LogType1)
 Log linear input: Input that is linear on a logarithmic scale (LogType2)
 Pseudo log input: An input that supports pseudo logs. (LogType2)
 Nonlinear log input: An input that supports nonlinear logs on which calibration correction (/CC1 option) is applied. Calibration correction is performed using voltage values. (LogType1)
 Range: 20 mV, 60 mV, 200 mV, 2 V, 6 V, 20 V, 50 V, and 1 V
 Unit symbol:
 Up to 6 characters in length
 Scalable range:
 Log input (LogType1)
 1.00E-15 to 1.00E+15 (15 decades maximum)
 Lower limit mantissa range: 1.00 to 9.99.
 Upper limit mantissa range: 1.00 to 9.99.
 Scale_L < Scale_U
 If the lower limit mantissa is 1.00, the difference between the exponents must be 1 or more.
 If the lower limit mantissa is a value other than 1.00, the difference between the exponents must be 2 or more.

Log linear input/Pseudo Log Input (LogType2)
 Lower limit mantissa range: 1.00 to 9.99. Upper limit mantissa range: N/A (the value is the same as the lower limit mantissa).
 If the lower limit mantissa is 1.00, the value must be between 1.00E-15 and 1.00E+15, the difference between the exponents must be 1 or more, and the maximum decades is 15.
 If the lower limit mantissa is a value other than 1.00, the value must be between 1.01E-15 and 9.99E+14, the difference between the exponents must be 1 or more and the maximum decades is 14.
 Alarm:
 Kind High limit, low limit, delay high limit, and delay low limit
 Range 1.00E-16 to 1.00E+16, mantissa: 1.00 to 9.99
 Hysteresis 0% (fixed)
 Color scale band range:
 1.00E-16 to 1.00E+16, mantissa: 1.00 to 9.99
 The display position lower limit must be less than the display position upper limit.
 Number of mantissa display digits: 2 or 3
 Type of LogType2: Select from Log linear or Pseudo Log.

15. Power Monitor (/PWR1)

Measurement element:
 By including power measurement elements in an expression, you can measure a variety of power values. Active power, regenerative electric power, reactive power, apparent power, voltage, current, frequency, power factor (LEAD: -, LAG: +), and electric energy (active energy, regenerative energy, reactive energy—LAG: +, reactive energy—LEAD: -, and apparent energy)
 * The LEAD/LAG sign is calculated from the phase difference between P1 (voltage) and I1 (current.)
 Phase and wiring system:
 Single-phase two-wire system, single-phase three-wire system, and three-phase three-wire system
 Frequency: 45 to 65 Hz
 Rated input voltage:

Rated Voltage	Voltage Range (Variable)	Allowable Input Voltage	Crest Factor
120 V	120 V	150 V	2
240 V	240 V	300 V	2

Rated input current:

Rated Current	Current Range (Fixed)	Allowable Input Current	Crest Factor
1 A	1 A	1.2 A	2

Allowable input range:
 150 Vrms (when the voltage range is set to 120 V), 300 Vrms (when the voltage range is set to 240 V), and 1.2 A (when using current input)

Rated input power and measuring range:
Single-phase two-wire system

Input (AC)	Rated Power	Input Measuring Range ¹	Approximate Consumed VA	
			Voltage	Current
120 V/1 A	100 W	-120 to 120 W	0.2 VA	0.2 VA
240 V/1 A	200 W	-240 to 240 W	0.4 VA	

Single-phase three-wire system

Input (AC)	Rated Power	Input Measuring Range	Approximate Consumed VA	
			Voltage	Current
200 V/1 A	200 W	-240 to 240 W	0.2 VA/Phase	0.2 VA/Phase

Three-phase three-wire system

Input (AC)	Rated Power	Input Measuring Range	Approximate Consumed VA	
			Voltage	Current
120 V/1 A	200 W	-240 to 240 W	0.2 VA/Phase	0.2 VA/Phase
240 V/1 A	400 W	-480 to 480 W	0.4 VA/Phase	

The input measuring range when you are using a VT and CT is calculated using the following equation. The measuring range must be within the input measuring ranges listed above, and the primary side input power² must be less than 10 GW.

- *1: Input measuring range (W) = Primary side input power in W²/(VT ratio × CT ratio).
- *2: Primary side input power = Secondary side rated power in W × 1.2 × VT ratio × CT ratio.

Measuring range:

Power factor: (LEAD) 0.5 to 1 to (LAG) 0.5

Frequency: 45 to 65 Hz

Measurement accuracy:

The performance values listed here were recorded under the following standard operating conditions: 23 ± 2°C, 55 ± 10%RH; power supply frequency: 50/60 Hz ± 1% or less; rated input: ±1% or less, power factor: 1 ± 1% or less; warm-up time: 30 minutes or more; and a location in which vibration and other factors do not affect the operation of the instrument.

Active power (W): ±1.0% of range

Voltage (V): ±1.0% of range

Current (A): ±1.0% of range

Apparent power, reactive power, and power factor:

Value calculated from the measured values ± 1 digit

Expressions (V and A are rms values)

	Apparent Power (VA)	Reactive Power (Q) (Without using the reactive power measurement method)	Power Factor(PF)
Single-phase two-wire system	$VA = V \times A$	$Q = \sqrt{((VA)^2 - P^2)}$	$\Sigma P / \Sigma VA$ (Without using the reactive power measurement method)
Single-phase, three-wire system	$VA_i = V_i \times A_i$ $i = 1, 2$ $\Sigma VA = VA1 + VA2$	$Q_i = \sqrt{((VA_i)^2 - P_i^2)}$ $i = 1, 2$ $\Sigma Q = Q1 + Q2$	
Three-phase three-wire system	$VA_i = V_i \times A_i$ $i = 1, 3$ $\Sigma VA = \sqrt{3}/2(VA1 + VA3)$	$Q_i = \sqrt{((VA_i)^2 - P_i^2)}$ $i = 1, 3$ $\Sigma Q = Q1 + Q3$	

* The FX's apparent power (VA), reactive power (Q), power factor (PF), and phase (deg) are determined from the voltage(V), current(A), and active power(P) by means of digital computations. Therefore, for distorted signal input, the value obtained on the FX may differ from that obtained on other instruments that use a different method.

* Make sure that the voltage input is at least 10% of the rated value and the current input is at least 5% of the rated value.

* In the ΣQ computation, each phase's Q value is computed as negative (-) if the current input is leading the voltage input and as positive (+) if the current input is lagging the voltage input.

Frequency: ±1.0 Hz

* The frequency of the voltage line input to voltage P1 is output in units of Hz.

Response time: 2 sec

Continuous overload:

Within the degree of accuracy (rated voltage and rated current × 1.2 applied for 2 hours)

Instantaneous overload:

Within the degree of accuracy (rated voltage × 1.5 applied for 10 seconds, rated current × 2 applied for 10 seconds, rated current × 10 applied for 3 seconds)

Dielectric strength:

2500 VAC (50/60 Hz) for 1 minute (between the current input, voltage input, and earth)

Insulation resistance:

100 MΩ (500 VDC between the current input, voltage input, and earth)

Computation functions:

The same as the computation function (/M1)

Effects of the operating conditions:

Ambient temperature

±0.05%/°C (under the following conditions: 0 to 50°C, 0.05 In ≤ I ≤ Imax, power factor = 1)

±0.07%/°C (under the following conditions: 0 to 50°C, 0.1 In ≤ I ≤ Imax, power factor = 0.5)

In: Rated current

Voltage variation

Within the degree of accuracy (90 to 132 VAC or 180 to 250 VAC; frequency is 50 or 60 Hz)

External magnetic fields

400 A/m or less

Active power and voltage: ±1.0% of range

Effect of the input frequency

For a change within 45 to 65 Hz, the effect on the active power, voltage, and current is within the accuracies.

■ General Specifications

1. Construction

- Mounting: Flush panel mounting (on a vertical plane)
 Mounting angle: Inclined backward up to 30 degrees from a horizontal plane.
 Allowable panel thickness: 2 to 26 mm
 Material Case: Metal plate
 Bezel and display cover: Polycarbonate
 Color Case: Grayish blue green (Munsell 2.0B5.0/1.7 or equivalent)
 Bezel: Charcoal gray light (Munsell 10B3.6/0.3 or equivalent)
 Front panel: Water and dust proof: Complies with IEC529-IP65, except side-by-side mounting
 External dimensions: 144 (W) × 144 (H) × 161.7 (D) mm (D: depth from the panel mounting plane)
 Weight: FX1002, FX1004, FX1006: 1.3 kg, FX1008, FX1010, FX1012: 1.4 kg, not including options

2. Normal Operating Conditions

- Supply voltage: 90 to 132, 180 to 250 VAC
 Power supply frequency: 50 Hz ± 2%, 60 Hz ± 2%
 Ambient temperature: 0 to 50°C
 Ambient humidity: 20 to 80%RH (at 5 to 40°C), 10 to 50% (at 40 to 50°C)
 Vibration: 10 to 60 Hz, 0.2 m/s²
 Shock: Not allowed
 Magnetic field: 400 A/m or less (DC and 50/60 Hz)
 Noise:
 Normal mode (50/60 Hz)
 DC voltage The peak value including the signal must be less than 1.2 times the measuring range.
 Thermocouple
 The peak value including the signal must be less than 1.2 times the measuring thermal electromotive force.
 RTD 50 mV or less
 Common mode noise
 250 VACrms or less for all ranges (50/60 Hz)
 Maximum noise voltage between channels
 FX1xxx-x-x-H: 250 VACrms (50 or 60 Hz) or less
 FX1xxx-x-x-L: 60 VACrms (50 or 60 Hz) or less
 Mounting position: Can be inclined up to 30 degrees backward. Left and right horizontal.
 Warm-up time: At least 30 minutes after power on
 Installation location: Indoors
 Operating altitude: 2000 m or less

3. Power Supply

- Rated supply voltage: 100 to 240 VAC
 Allowable power supply voltage range: 90 to 132, 180 to 264 VAC
 Rated power supply frequency: 50 Hz, 60 Hz

Power consumption:

Supply voltage	LCD backlight off	Normal	Maximum
100 VAC	10 VA	15 VA	35 VA
240 VAC	15 VA	20 VA	45 VA

Allowable interruption time:

Less than 1 cycle of the power supply frequency

4. Isolation

Insulation resistance:

Between the Ethernet, RS-422A/485, and insulation terminals and earth: 20 MΩ or greater at 500 VDC

Withstand voltage:

Between the power terminal and earth: 2300 VAC at 50/60 Hz for one minute

Between the contact output terminal and earth: 1600 VAC at 50/60 Hz for one minute

Between the measurement input terminal and earth: 1500 VAC at 50/60 Hz for one minute

Between the measurement input terminals (excluding the RTD input terminal of the FX1006, FX1008, FX1010, FX1012):

FX1xxx-x-x-H: 1000 VAC (50 or 60 Hz) for 1 minute

FX1xxx-x-x-L: 400 VAC (50 or 60 Hz) for 1 minute

Between the remote input terminal and earth: 1000 VDC for one minute

Between the pulse input terminal and earth: 1000 VDC for one minute

Between the power monitor input terminals (current input, voltage input, and earth): 2500 VAC (50 or 60 Hz) for 1 minute

Ground: Grounding resistance: 100 Ω or less

5. Transport and Storage Conditions

Ambient temperature: -25 to 60°C

Ambient humidity: 5 to 95%RH (no condensation)

Vibration: 10 to 60 Hz, 4.9 m/s² maximum

Shock: 392 m/s² maximum (in packaged condition)

6. Supported Standards

- CSA: CSA22.2 No.61010-1, CSA C22.2 No. 61010-2-030, installation category II^{*1} and pollution degree 2^{*2}
- UL: UL61010-1, UL61010-2-030 (CSA NRTL/C)
- CE:
EMC directive
EN61326-1 compliance, Class A, Table 2 (For use in industrial locations)
EN61000-3-2 compliance
EN61000-3-3 compliance
EN55011 compliance, Class A, Group 1
- Low voltage directive
EN61010-1, EN61010-2-030, installation category II^{*1} and pollution degree 2^{*2}

EMC Regulatory Arrangement in Australia and New Zealand
EN55011 compliance, Class A, Group 1

- *1: Installation category (overvoltage category) II: Describes a number which defines a transient overvoltage condition. Implies the regulation for impulse withstand voltage. "II" applies to electrical equipment which is supplied from the fixed installation like a distribution board.
- *2: Pollution degree 2: Describes the degree to which a solid, liquid, or gas which deteriorates dielectric strength or surface resistivity is adhering. "2" applies to normal indoor atmosphere. Normally, only non-conductive pollution occurs.

7. Standard Performance

- Measurement/display accuracy:
Standard operating conditions:
Temperature: 23 ± 2°C
Humidity: 55% ± 10%RH
Power supply voltage: 90 to 132 or 180 to 250 VAC
Power supply frequency: 50/60 Hz ± 1%
Warm-up time: At least 30 minutes.
Other ambient conditions such as vibration should not adversely affect the operation.

Input Type	Range	Measurement Accuracy (Digital display)	Digital Display Max. Resolution
DC voltage	20 mV	±(0.05% of rdg + 12 digits)	1 μV
	60 mV	±(0.05% of rdg + 3 digits)	10 μV
	200 mV		10 μV
	1 V		100 μV
	2 V	±(0.05% of rdg + 12 digits)	100 μV
	1 to 5 V	±(0.05% of rdg + 3 digits)	1 mV
	6 V		1 mV
	20 V		1 mV
	50 V		10 mV
Thermocouple (Not including the accuracy of reference junction compensation; when the burnout detection function is off.)	R	±(0.15% of rdg + 1°C) R, S: 0 to 100°C: ±3.7°C, 100 to 300°C: ±1.5°C B: 400 to 600°C: ±2°C; accuracy not guaranteed for temperatures less than 400°C	0.1°C
	S		
	B		
	K	±(0.15% of rdg + 0.7°C) -200 to -100°C: ±(0.15% of rdg + 1°C)	
	E	±(0.15% of rdg + 0.5°C) -200 to -100°C: ±(0.15% of rdg + 0.7°C)	
	J		
	T		
	N	±(0.15% of rdg + 0.7°C) -200 to 0°C: ±(0.35% of rdg + 0.7°C) Accuracy not guaranteed for values less than -200°C.	
	W	±(0.15% of rdg + 1°C)	
	L	±(0.15% of rdg + 0.5°C) -200 to -100°C: ±(0.15% of rdg + 0.7°C)	
	U		
WRe	±(0.2% of rdg + 2.5°C) 0 to 200°C: ±4.0°C		
RTD	Pt100	±(0.15% of rdg + 0.3°C)	
	JPt100		
DI	Voltage	Threshold level (V _{th} =2.4 V) accuracy ± 0.1 V	
	Contact	With parallel capacitance of 0.01 μF or less, 1 kΩ or less: 1 (ON). 100 kΩ or more: 0 (OFF)	

Measuring accuracy in case of scaling
 Accuracy during scaling (digits) =
 measurement accuracy (digits) ×
 multiplier + 2 digits (rounded up)

* Fractions rounded up
 where the multiplier = scaling span (digits)/
 measuring span (digits).

Example For 1-5 V range (A/D integration time is
 16.7 ms or more), measurement span
 of 1.000 to 5.000 V, and scaling span of
 0.000 to 2.000
 The measuring accuracy for 5 V input is
 as follows.
 Measuring accuracy (1-5 V range)
 = $\pm(0.05\% \times 5 \text{ V} + 3 \text{ digits}) = \pm(0.0025 \text{ V}$
 $[3 \text{ digits}] + 3 \text{ digits}) = \pm 6 \text{ digits}$
 Multiplier = $\{2000 \text{ digits} (0.000 \text{ to}$
 $2.000)\} / 4000 \text{ digits} (1.000 \text{ to } 5.000) =$
 0.5
 Thus, accuracy during scaling = $\pm(6 \times$
 $0.5 + 2) \text{ digits} = 5 \text{ digits (rounded up)}$

Reference junction compensation accuracy:
 When measuring temperature
 greater than or equal to 0 °C and
 when input terminal temperature is
 balanced

Type R, S, W, and WR: $\pm 1.0^\circ\text{C}$
 Type K, J, E, T, N, L, and U: $\pm 0.5^\circ\text{C}$.

Type B: Internal reference compensation is fixed
 to 0°C

Maximum input voltage: $\pm 60 \text{ VDC}$ (continuous)

Input resistance:
 1 V range or less and TC: 10 M Ω or more
 2 V range or higher: Approx. 1 M Ω

Input source resistance:
 Volt, TC 2 k Ω or less
 RTD input 10 Ω or less per wire (The resistance of
 all three wires must be equal).

Bias current:
 10 nA or less (except when burnout
 detection function is enabled)

Maximum common mode noise voltage:
 250 VACrms (50 Hz/60 Hz)

Maximum noise voltage between channels:
 FX1xxx-x-x-H 250VACrms (50/60Hz)
 FX1xxx-x-x-L 60VACrms (50/60Hz)

Interference across channels:
 120 dB (when the input source resistance
 is 500 Ω and the input to other channels is
 60 VDC)

Common mode rejection ratio:
 When the A/D integration time is 20 ms
 120 dB (50 Hz $\pm 0.1\%$, 500 Ω
 unbalanced, between the minus terminal
 and ground)
 When the A/D integration time is 16.7 ms
 120 dB (60 Hz $\pm 0.1\%$, 500 Ω
 unbalanced, between the minus terminal
 and ground)

Normal mode rejection ratio:
 When the A/D integration time is 20 ms
 40 dB or more (50 Hz $\pm 0.1\%$)
 When the A/D integration time is 16.7 ms
 40 dB or more (60 Hz $\pm 0.1\%$)

8. Effects of Operating Conditions

Ambient temperature (with temperature variation of
 10°C):
 DC voltage, TC range
 $\pm(0.1\% \text{ of rdg} + 0.05\% \text{ of range})$ or less

* Excluding the error of reference junction
 compensation

RTD range
 $\pm(0.1\% \text{ of rdg} + 2 \text{ digits})$ or less

Power supply fluctuation
 With variation within 90 to 132 V and 180
 to 250 VAC (50/60 Hz):
 Accuracy specifications are satisfied.
 With variation of $\pm 2 \text{ Hz}$ from rated
 power frequency (power supply voltage
 100 VAC): Accuracy specifications are
 satisfied.

Magnetic field:
 AC (50/60 Hz) and DC 400 A/m fields:
 $\pm(0.1\% \text{ of rdg} + 10 \text{ digits})$ or less

Input source resistance:
 DC voltage range
 With variation of +1 k Ω :
 1 V range or less: $\pm 10 \mu\text{V}$ or less
 2 V range or higher: $\pm 0.15\%$ of rdg or less
 TC range
 With variation of +1 k Ω : $\pm 10 \mu\text{V}$ or less

RTD range (Pt100)
 With variation of 10 Ω per wire
 (resistance of all three wires must be
 equal): $\pm(0.1\% \text{ of rdg} + 1 \text{ digits})$ or less
 With maximum difference of 40 m Ω
 between wires: Approx. 0.1 °C

Effects of vibration:
 Effects from a sinusoidal vibration along
 all three axis at a frequency between 10
 to 60 Hz and an acceleration of 0.2 m/s²:
 $\pm(0.1\% \text{ of rdg} + 1 \text{ digit})$ or less

9. Miscellaneous

Memory backup:
 A built-in lithium battery backs up the
 settings and runs the clock
 Battery life: Approximately 10 years (at
 room temperature)

■ Application Software

1. Operating environment

Operating System (OS):

Windows XP

Home Edition SP3
Professional SP3 (excluding 64-bit Editions)

Windows Vista

Home Premium SP2 (excluding 64-bit editions)
Business SP2 (excluding 64-bit editions)

Windows 7

Home Premium, SP1 (32- or 64-bit edition)
Professional, SP1 (32- or 64-bit edition)

CPU and Main Memory:

When Using Windows XP

Pentium III, 600 MHz or faster Intel x64 or x86 processor; 128 MB or more of memory

When Using Windows Vista

Pentium 4, 3 GHz or faster Intel x64 or x86 processor; 2 GB or more of memory

When Using Windows 7

32-bit edition: Intel Pentium 4, 3 GHz or faster x64 or x86 processor; 2 GB or more of memory
64-bit edition: Intel x64 processor that is equivalent to Intel Pentium 4, 3 GHz or faster; 2 GB or more of memory

Hard Disk:

A free space of 100 MB or more (more space may be required, depending on the amount of data stored).

CD-ROM Drive:

To be used for installing the software.

Mouse: A mouse supported by Windows.

Monitor: A video card that is recommended for the OS and a display that is supported by the OS, has a resolution of 1024×768 or higher, and that can show 65,536 colors (16-bit, high color) or more.

Printer: A printer supported by Windows is required. An appropriate printer driver is also required.

Adobe Reader: Adobe Reader 7 or later

2. Configuration software:

Setting mode:

Configuration of setting mode and basic setting mode

Configuration via communication:

Configuration of setting mode and basic setting mode without communication configuration (ex. IP address)

3. Data viewer software:

Number of display channels:

32 channels per group, 50 groups maximum

Viewer function:


Waveform display, digital display, circular display, list display, report display, etc.

Data conversion:


File conversion to ASCII, Lotus 1-2-3 or MS-Excel format

■ Dimensions

External dimensions


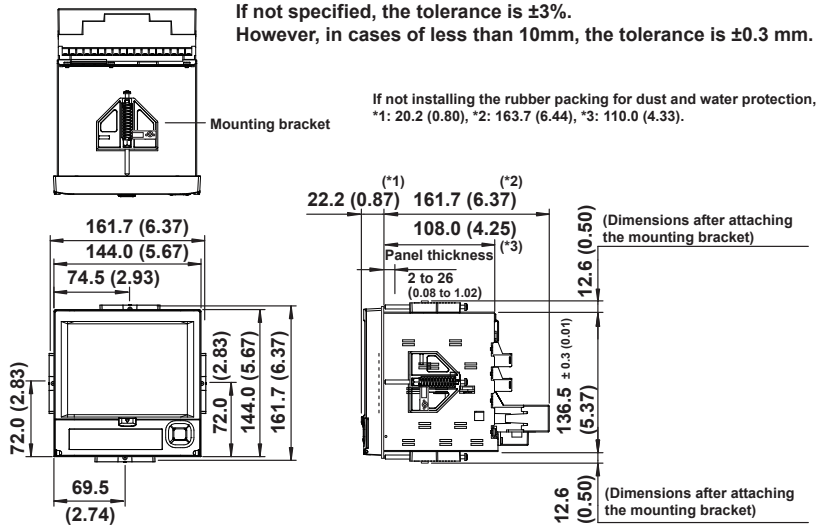


Panel cut dimensions

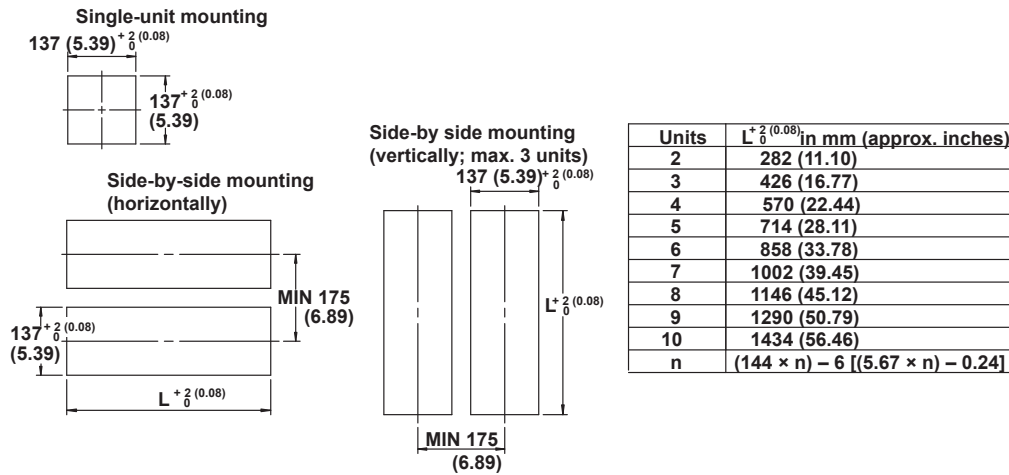



■ Arrangement of the Terminals

1. Input Terminals

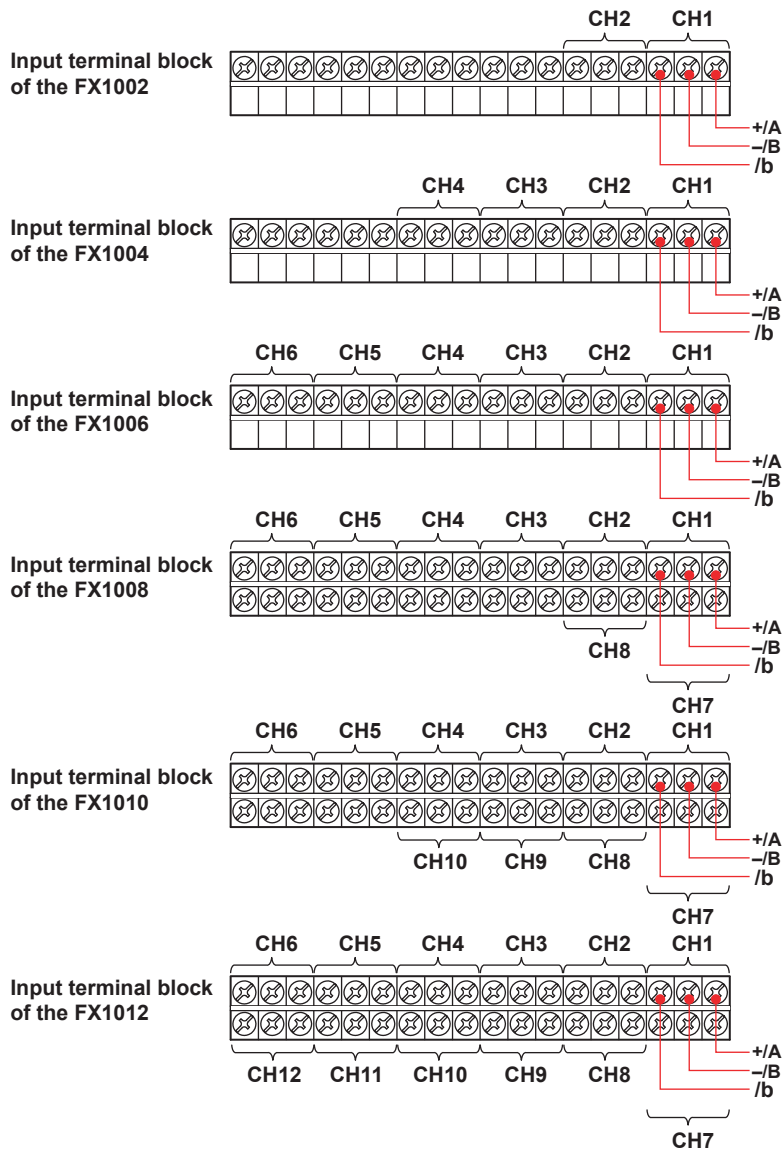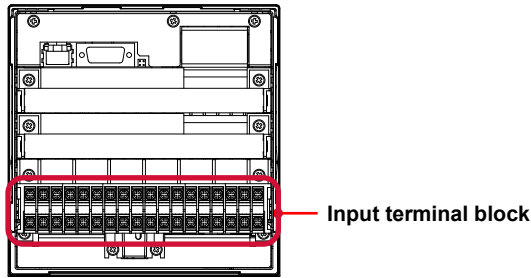

For TC input, use shielded compensating lead wires for wiring.
For RTD input, lead wire resistance per wire of 10 Ω or less. Make the resistances of the three wires equal.
For DCA input, example: for 4 to 20 mA input, use a shunt resistor of 250 Ω ± 0.1%.

2. Optional Terminals

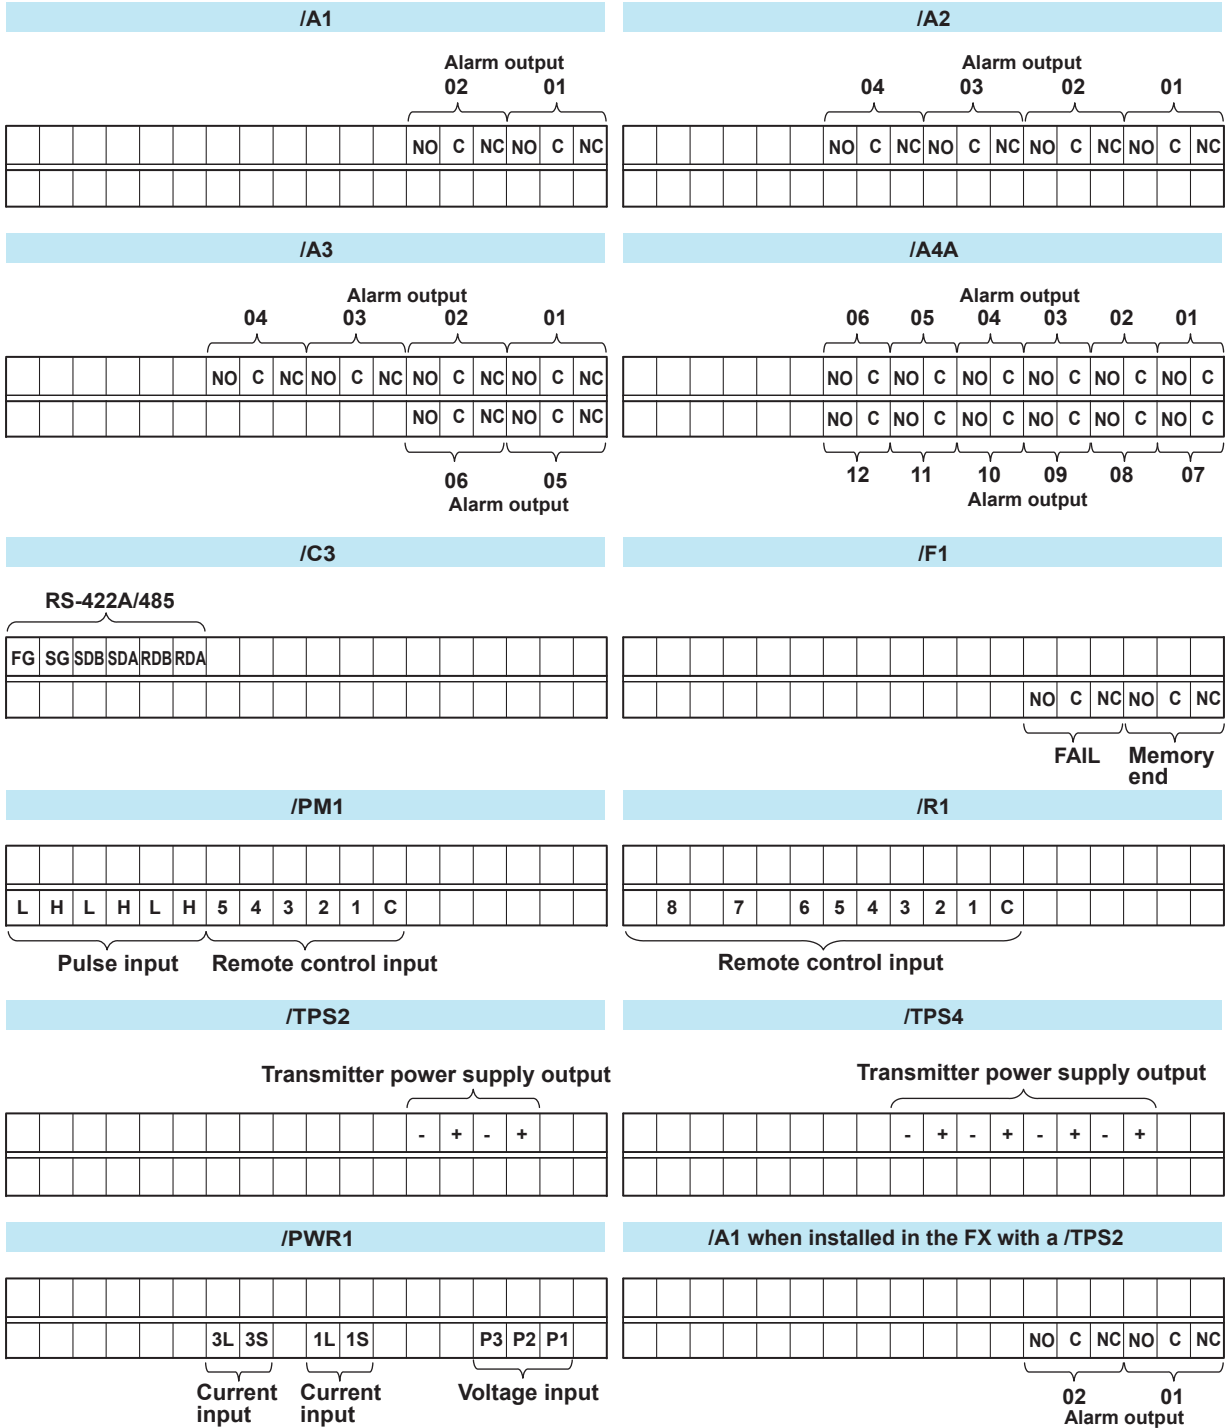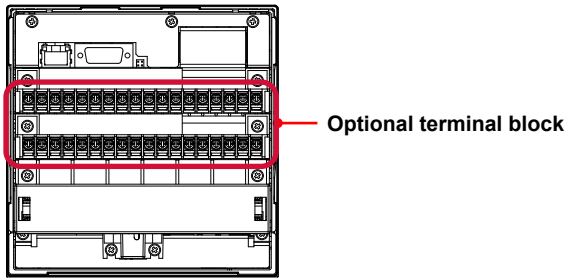

■ Model and Suffix Code

Model code	Suffix code	Optional code	Description
FX1002			2ch, Shortest measurement interval: 125ms
FX1004			4ch, Shortest measurement interval: 125ms
FX1006			6ch, Shortest measurement interval: 1s
FX1008			8ch, Shortest measurement interval: 1s
FX1010			10ch, Shortest measurement interval: 1s
FX1012			12ch, Shortest measurement interval: 1s
External storage medium slot	-0		Without CF card slot and medium ^(Note)
	-4		With CF card slot and medium
Language	-2		English/Japanese/German/French/Chinese/Italian/Spanish/Portuguese/Russian/Korean, deg F and DST
Withstanding voltage between measuring input terminals		-H	1000 VAC(50/60 Hz), 1 min
		-L	400 VAC(50/60 Hz), 1 min
Options		/A1	Alarm output 2 points (C-contact) ^{*10}
		/A2	Alarm output 4 points (C-contact) ^{*1}
		/A3	Alarm output 6 points (C-contact) ^{*13}
		/A4A	Alarm output 12 points (A-contact) ^{*13}
		/C2	RS-232 interface ^{*2}
		/C3	RS-422A/485 interface ^{*2}
		/C7	Ethernet interface
		/F1	FAIL/Status output ^{*3}
		/M1	Mathematical functions (including Report functions)
		/N2	3 leg isolated RTD ^{*4}
		/N3F	Extended input type (without Pt1000)
		/P1	24 VDC/AC power supply
		/R1	Remote control 8 points ^{*5}
		/TPS2	24VDC transmitter power supply (2 loops) ^{*6*10}
		/TPS4	24VDC transmitter power supply (4 loops) ^{*7}
		/USB1	USB interface (1 port)
	/PM1	Pulse input 3 points, Remote control 5 points (including Mathematical functions) ^{*8}	
	/CC1	Calibration correction function	
	/LG1	Log scale	
	/PWR1	Power monitor (including Mathematical functions) ^{*9*10}	

Note: To load data, the FX must be equipped with a communication interface (/C2, /C3, or /C7 option) or the USB interface (/USB1 option).

*1 Any combination of /A1, /A2, /A3, and /A4A cannot be specified together.

*2 /C2 and /C3 cannot be specified together.

*3 /A3 or /A4A cannot be specified together with /F1.

*4 /N2 cannot be specified for FX1002 or FX1004.

*5 If /R1 is specified, /A4A, /TPS2, /TPS4, /PM1, or /PWR1 cannot be specified.

*6 If /TPS2 is specified, /TPS4, /A2, /A3, /A4A, /F1, /R1, or /PM1 cannot be specified.

*7 If /TPS4 is specified, /TPS2, /A1, /A2, /A3, /A4A, /F1, /R1, or /PM1 cannot be specified.

*8 If /PM1 is specified, /A4A, /M1, /R1, /TPS2, /TPS4, or /PWR1 cannot be specified.

*9 If /PWR1 is specified, /A3, /A4A, /F1, /R1, /PM1, or /M1 cannot be specified.

*10 /TPS2, /PWR1, and /A1 cannot be specified together.

Precaution on purchasing the Log scale (Optional code, /LG1)

To support the nonlinear output of vacuum gauges, the FX must be required with the Log scale (/LG1) and the calibration correction function (/CC1).

Model code	Description
FXA120	DAQSTANDARD software

* DAQSTANDARD software (R9.02.01 or earlier) does not support the pseudo log and nonlinear log settings of the FX1000.

■ Standard Accessories

Name	Model	Qty.	Notes
Mounting brackets	B8730BU	2	For panel mounting
Rubber packing for dust and water protection	-	1	For single-unit mounting
FX1000 DAQSTANDARD/Manuals	FXA120	1	CD. Contains the software and user's manuals.
FX1000 Safety Precautions and Installation Guide	IM 04L21B01-03EN	1	A3 size
How to Use the CD Installing FXA120 DAQSTANDARD and Opening FX1000 Manuals	IM 04L21B01-66EN	1	A4 size
CF card ^{*1}	772093	1	512 MB

*1 On FXs that have a CF card slot (suffix code -4.)
CF card capacity is subject to change.

■ Optional Accessories (Sold Separately)

Name	Model	Q'ty	Notes
CF card	772093	1	512 MB
	772094	1	1 GB
	772095	1	2 GB
CF card adapter	772090	1	-
Shunt resistor	X010-250-3	1	250 Ω ± 0.1%
	X010-100-3	1	100 Ω ± 0.1%
	X010-010-3	1	10 Ω ± 0.1%
Mounting brackets	B8730BU	2	-
Terminal screws	B8730CZ	-	M3 (spares for I/O terminals)
	B8730CY	-	M4 (spares for power terminals)

- The TCP/IP software of this product and the document concerning the TCP/IP software have been developed/ created by YOKOGAWA based on the BSD Networking Software, Release 1 that has been licensed from the Regents of the University of California.
- FX1000 and DAQSTANDARD are registered trademarks or trademarks of Yokogawa Electric Corporation.
- Microsoft and Windows are registered trademarks or trademarks of Microsoft Corporation in the United States and/ or other countries.
- Lotus and 1-2-3 are registered trademarks of Lotus Development Corporation.
- Pentium is a registered trademark of Intel Corporation.
- Ethernet is a registered trademark of XEROX Corporation.
- Modbus is a registered trademark of AEG Schneider.
- Adobe Reader is a registered trademark or trademark of Adobe Systems Incorporated.
- Company and product names that appear in General Specification are registered trademarks or trademarks of their respective holders.
- The company and product names used in General Specification are not accompanied by the registered trademark or trademark symbols (® and ™.)